


Shored Mechanically Stabilized Earth (SMSE) Wall Systems Design Guidelines

Publication No. FHWA-CFL/TD-06-001

February 2006

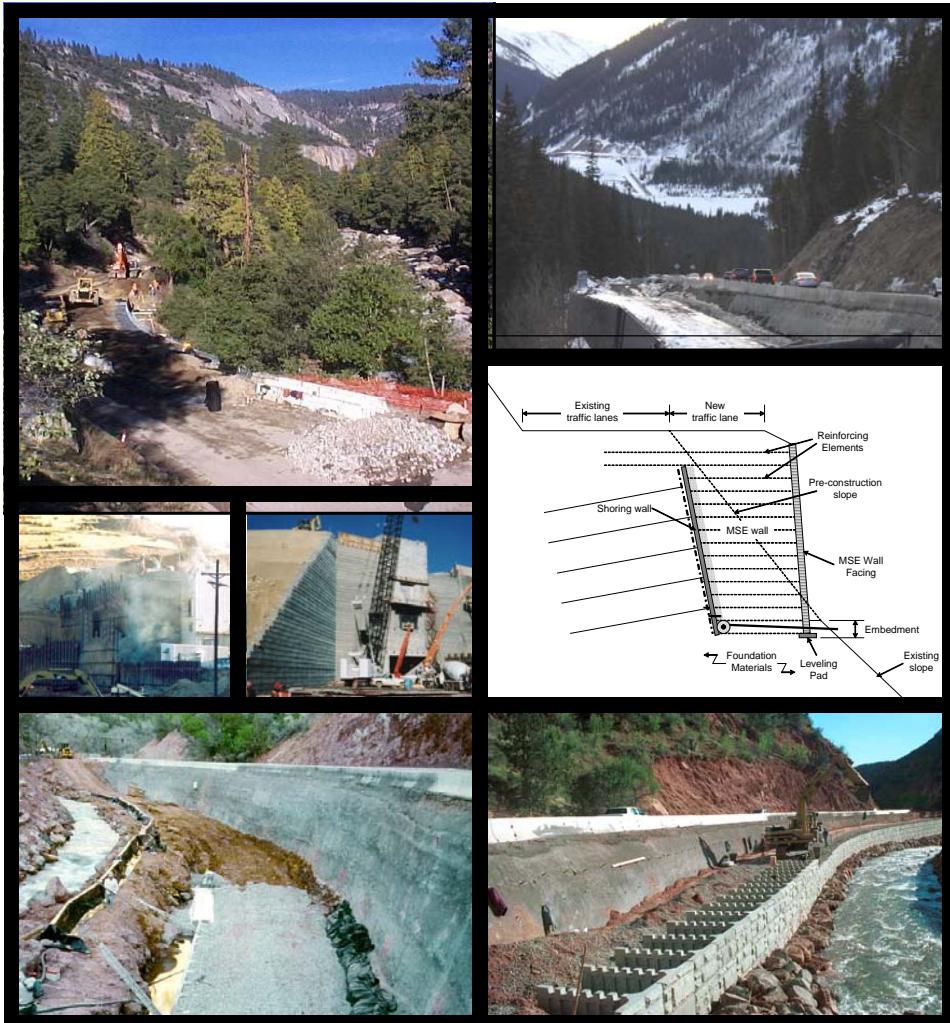

U.S. Department
of Transportation

Federal Highway
Administration



Central Federal Lands Highway Division
12300 West Dakota Avenue
Lakewood, CO 80228

FOREWORD

Federal Lands Highway (FLH) is responsible for design and construction of roadways in rugged, mountainous terrain. MSE walls are frequently used to accommodate widening of existing roads or construction of new roadways. However, in steep terrain, excavation is required to establish a flat bench on which to construct the MSE wall.

Shoring has often been employed to stabilize the backslope (or back-cut) for the MSE wall, and an MSE wall has been designed and constructed in front of it. Where a shored MSE wall system is determined to be the best alternative for wall construction, design of the MSE wall component should take into consideration the retaining benefits provided by the shoring component, as well as the long-term behavior of each individual wall system. The purpose of this design guideline is to serve as the FLH standard reference for highway projects involving shored MSE walls.

Notice

This document is disseminated under the sponsorship of the U.S. Department of Transportation in the interest of information exchange. The U.S. Government assumes no liability for the use of the information contained in this document. This report does not constitute a standard, specification, or regulation.

The U.S. Government does not endorse products or manufacturers. Trademarks or manufacturers' names appear in this report only because they are considered essential to the objective of the document.

Quality Assurance Statement

The Federal Highway Administration (FHWA) provides high-quality information to serve Government, industry, and the public in a manner that promotes public understanding. Standards and policies are used to ensure and maximize the quality, objectivity, utility, and integrity of its information. FHWA periodically reviews quality issues and adjusts its programs and processes to ensure continuous quality improvement.

Technical Report Documentation Page

1. Report No. FHWA-CFL/TD-06-001	2. Government Accession No.	3. Recipient's Catalog No.	
4. Title and Subtitle <i>Shored Mechanically Stabilized Earth (SMSE) Wall Systems Design Guidelines</i>		5. Report Date February 2006	
		6. Performing Organization Code 023-2436	
7. Author(s) Kimberly Finke Morrison, P.E., R.G.; Francis E. Harrison, P.E.; James G. Collin, Ph.D., P.E.; Andrew Dodds, Ph.D.; and Ben Arndt, P.E.		8. Performing Organization Report No.	
9. Performing Organization Name and Address Golder Associates Inc. The Collin Group, Ltd. Yeh and Associates, Inc. 44 Union Blvd., Suite 300 7445 Arlington Road 5700 E. Evans Ave Lakewood, CO 80228 Bethesda, MD 20814 Denver, CO 80222		10. Work Unit No. (TRAIS)	
		11. Contract or Grant No. DTFH68-02-R-00001	
12. Sponsoring Agency Name and Address Federal Highway Administration Central Federal Lands Highway Division 12300 W. Dakota Avenue, Suite 210 Lakewood, CO 80228		13. Type of Report and Period Covered Final, Oct. 2002 – Feb. 2006	
		14. Sponsoring Agency Code HFTS-16.4	
15. Supplementary Notes Contracting Officer's Technical Representative (COTR): Scott A. Anderson, Ph.D., P.E., FHWA-FLH; Advisory Panel Members: Mike Adams, FHWA-TFHRC; Rich Barrows, FHWA-WFLHD; and Daniel Alzamora and Roger Surdahl, FHWA-CFLHD. This project was funded under the FHWA Federal Lands Highway Coordinated Technology Implementation Program (CTIP).			
16. Abstract As an FHWA design reference for highway projects, this report was prepared to enable the engineer to identify and evaluate potential applications of shored mechanically stabilized earth (SMSE) walls. Included in this design guideline are a literature review on similar construction and the results and interpretation of field-scale testing, centrifuge modeling, and numerical modeling of an SMSE wall system. Results of the centrifuge modeling and field-scale testing show that reduction of the reinforcement length to as little as 25 percent of the wall height ($0.25H$) provides sufficient wall stability, even under a considerably high degree of surcharge loading.			
Using the results of the modeling and field testing research, this design guideline recommends a minimum reinforcement length equivalent to as little as 30 percent of the wall height ($0.3H$) for the MSE wall component, provided that the MSE reinforcement length is greater than 1.5 m. The benefit of attaching reinforcement to the shoring wall is found to be small and is generally not recommended except by way of the upper two layers of reinforcement. If possible, these layers of reinforcement should overlap the shoring wall and have a total length of $0.6H$. If this is not possible, then these layers should be attached to the shoring wall.			
Internal design requirements of the MSE wall component for an SMSE wall system differ from that of a traditional MSE wall. Equations presented in this design guideline have been developed specifically to address these requirements. The benefits of increased retaining abilities provided by the shoring wall, such as reduction in lateral load acting on the MSE wall component and contribution to global stability, are considered in the design process.			
17. Key Words DESIGN, MECHANICALLY STABILIZED EARTH (MSE) WALLS, SHORING WALLS, RETAINING WALLS, HIGHWAY CONSTRUCTION, HIGHWAY WIDENING		18. Distribution Statement No restriction. This document is available to the public from the sponsoring agency at the Website: http://www.cflhd.gov .	
19. Security Classif. (of this report) Unclassified	20. Security Classif. (of this page) Unclassified	21. No. of Pages 230	22. Price

SI* (MODERN METRIC) CONVERSION FACTORS					
APPROXIMATE CONVERSIONS TO SI UNITS					
Symbol	When You Know	Multiply By	To Find	Symbol	
		LENGTH			
in	inches	25.4	millimeters	mm	
ft	feet	0.305	meters	m	
yd	yards	0.914	meters	m	
mi	miles	1.61	kilometers	km	
		AREA			
in ²	square inches	645.2	square millimeters	mm ²	
ft ²	square feet	0.093	square meters	m ²	
yd ²	square yard	0.836	square meters	m ²	
ac	acres	0.405	hectares	ha	
mi ²	square miles	2.59	square kilometers	km ²	
		VOLUME			
fl oz	fluid ounces	29.57	milliliters	mL	
gal	gallons	3.785	liters	L	
ft ³	cubic feet	0.028	cubic meters	m ³	
yd ³	cubic yards	0.765	cubic meters	m ³	
NOTE: volumes greater than 1000 L shall be shown in m ³					
		MASS			
oz	ounces	28.35	grams	g	
lb	pounds	0.454	kilograms	kg	
T	short tons (2000 lb)	0.907	megagrams (or "metric ton")	Mg (or "t")	
		TEMPERATURE (exact degrees)			
°F	Fahrenheit	5 (F-32)/9 or (F-32)/1.8	Celsius	°C	
		ILLUMINATION			
fc	foot-candles	10.76	lux	lx	
fl	foot-Lamberts	3.426	candela/m ²	cd/m ²	
		FORCE and PRESSURE or STRESS			
lbf	poundforce	4.45	newtons	N	
lbf/in ²	poundforce per square inch	6.89	kilopascals	kPa	
APPROXIMATE CONVERSIONS FROM SI UNITS					
Symbol	When You Know	Multiply By	To Find	Symbol	
		LENGTH			
mm	millimeters	0.039	inches	in	
m	meters	3.28	feet	ft	
m	meters	1.09	yards	yd	
km	kilometers	0.621	miles	mi	
		AREA			
mm ²	square millimeters	0.0016	square inches	in ²	
m ²	square meters	10.764	square feet	ft ²	
m ²	square meters	1.195	square yards	yd ²	
ha	hectares	2.47	acres	ac	
km ²	square kilometers	0.386	square miles	mi ²	
		VOLUME			
mL	milliliters	0.034	fluid ounces	fl oz	
L	liters	0.264	gallons	gal	
m ³	cubic meters	35.314	cubic feet	ft ³	
m ³	cubic meters	1.307	cubic yards	yd ³	
		MASS			
g	grams	0.035	ounces	oz	
kg	kilograms	2.202	pounds	lb	
Mg (or "t")	megagrams (or "metric ton")	1.103	short tons (2000 lb)	T	
		TEMPERATURE (exact degrees)			
°C	Celsius	1.8C+32	Fahrenheit	°F	
		ILLUMINATION			
lx	lux	0.0929	foot-candles	fc	
cd/m ²	candela/m ²	0.2919	foot-Lamberts	fl	
		FORCE and PRESSURE or STRESS			
N	newtons	0.225	poundforce	lbf	
kPa	kilopascals	0.145	poundforce per square inch	lbf/in ²	

*SI is the symbol for the International System of Units. Appropriate rounding should be made to comply with Section 4 of ASTM E380.
(Revised March 2003)

TABLE OF CONTENTS

EXECUTIVE SUMMARY	1
CHAPTER 1 — INTRODUCTION	3
1.1 BACKGROUND	3
1.2 OBJECTIVE	3
1.2.1 Scope	4
1.2.2 Source Documents	5
1.2.3 Terminology	5
1.3 PRELIMINARY RESULTS.....	6
CHAPTER 2 — EVALUATION OF SMSE WALL SUITABILITY	7
2.1 PRE-DECISION EVALUATION STUDIES.....	7
2.1.1 MSE Feasibility Assessment	7
2.1.2 Determination of Shoring Requirements	9
2.1.3 Feasibility Design of SMSE Wall System.....	9
2.2 DECISION POINT	10
2.2.1 FHWA Experience with SMSE Walls	10
2.2.2 SMSE Wall Selection Process.....	12
CHAPTER 3 — SMSE WALL DESIGN BASIS	15
3.1 SMSE WALL RESEARCH REVIEW	15
3.1.1 Literature Review Summary.....	15
3.1.2 Centrifuge Modeling Summary	15
3.1.3 Field-Scale Test Summary	16
3.1.4 Numerical Modeling Summary	17
3.2 APPLICATION OF RESEARCH RESULTS TO DESIGN OF SMSE WALLS	17
3.3 SMSE WALL DESIGN CONSIDERATIONS	19
3.3.1 Backfill Selection	19
3.3.2 Geometric Considerations	21
3.3.3 Drainage Considerations	28
CHAPTER 4 — SITE INVESTIGATION OVERVIEW	29
4.1 FIELD RECONNAISSANCE	29
4.2 GEOTECHNICAL INVESTIGATION	29
CHAPTER 5 — DESIGN OF MSE WALL COMPONENT.....	33
5.1 POTENTIAL FAILURE MODES	34
5.1.1 Global Failure	34
5.1.2 Compound Failure of Shoring System and Foundation	34
5.1.3 Failure Across Interface	35
5.1.4 Interface Shear Failure	35
5.1.5 Compound Failure of MSE Wall and Foundation	35
5.1.6 Internal Failure of the MSE Wall	35

5.2 FACTORS OF SAFETY	36
5.3 INTERNAL STABILITY DESIGN	36
5.4 EXTERNAL STABILITY DESIGN	48
5.4.1 Bearing Capacity	48
5.4.2 Settlement	51
5.5 GLOBAL STABILITY DESIGN	52
5.5.1 General	52
5.5.2 MSE Wall/Shoring Interface	54
5.5.3 External to SMSE Wall System	57
5.6 SEISMIC STABILITY	58
5.7 CONNECTION STRENGTH DESIGN	59
5.8 MSE WALL BEHAVIOR	59
 CHAPTER 6 — SHORING COMPONENT DESIGN CONSIDERATIONS.....	61
6.1 COMMON TYPES OF SHORING WALLS	61
6.2 SOIL NAIL WALL DESIGN FOR SMSE WALLS.....	62
6.3 SHORING WALL BEHAVIOR	64
 CHAPTER 7 — DESIGN EXAMPLE.....	67
7.1 INTERNAL STABILITY DESIGN	67
7.2 EXTERNAL STABILITY DESIGN	70
7.2.1 Bearing Capacity Check	70
7.2.2 Settlement Check	71
7.3 GLOBAL STABILITY DESIGN	71
7.3.1 MSE Wall/Shoring Interface Stability Check	71
7.3.2 Stability External to SMSE Wall System	72
 CHAPTER 8 — PROCUREMENT AND CONSTRUCTABILITY ISSUES.....	77
8.1 PROCUREMENT ISSUES	77
8.1.1 General	77
8.1.2 SCR Considerations.....	78
8.2 CONSTRUCTABILITY ISSUES	79
8.2.1 Confined Space for MSE Fill	79
8.2.2 Reinforcement Connections and Overlaps	79
8.2.3 Rock or Difficult Excavation.....	79
8.2.4 Geometric Tolerances.....	80
8.2.5 Foundation Preparation	80
8.2.6 Interface Friction	80
8.2.7 Groundwater	81
 CHAPTER 9 — CONCLUSIONS AND RECOMMENDATIONS	83
9.1 CONCLUSIONS	83
9.2 RECOMMENDATIONS.....	84
9.2.1 Implementation.....	85

9.2.2 Wall Monitoring	85
9.2.3 Future Research.....	87
APPENDIX A — LITERATURE REVIEW.....	89
A.1 REINFORCEMENT SPACING	89
A.2 REINFORCEMENT LENGTH	89
A.2.1 Geosynthetic-Reinforced Soil Retaining Walls.....	90
A.2.2 Constrained Reinforced Fill Zones.....	91
A.2.3 Other Constructed Cases of Short Reinforcement Lengths	92
A.2.4 Numerical Analyses Evaluating Short Reinforcement Lengths	94
A.2.5 Summary.....	95
A.3 NON-RECTANGULAR REINFORCEMENT GEOMETRY	95
A.3.1 North American Practice	95
A.3.2 European Practice	97
A.3.3 Asian Practice	97
A.4 DESIGN EARTH PRESSURES	97
A.4.1 North American Practice	97
A.4.2 European Practice	98
A.4.3 Asian Practice	98
A.5 FULL-SCALE TESTING OF MSE WALLS.....	99
A.6 PERTINENT LITERATURE REVIEW FINDINGS.....	101
APPENDIX B — CENTRIFUGE MODELING OF SHORED MSE WALL	103
B.1 CENTRIFUGE MODELING	103
B.2 MODELING PARAMETERS	103
B.2.1 Materials	103
B.2.2 Testing Apparatus	106
B.3 TESTING PROGRAM	107
B.3.1 Phase I.....	108
B.3.2 Phase II	108
B.4 RESULTS	112
B.4.1 Phase I.....	112
B.4.2 Phase II	116
APPENDIX C — FIELD-SCALE TESTING OF SMSE WALL.....	119
C.1 PURPOSE	119
C.2 TEST WALL DESIGN	119
C.3 TEST WALL CONSTRUCTION.....	122
C.4 INSTRUMENTATION AND MONITORING	127
C.5 WALL LOADING	132
C.6 RESULTS	134
C.6.1 Visual Observations.....	134
C.6.2 Strain Gages	134
C.6.3 Pressure Cells.....	137
C.6.4 Inclinometer Measurements.....	142
C.6.5 Survey Measurements.....	144

C.6.6 LVDT Measurements	147
C.6.7 Potentiometer Measurements.....	148
C.7 INSTRUMENTATION SUMMARY	149
C.8 COMPARISON OF CENTRIFUGE AND FIELD-SCALE MODELING	150
C.9 FACTOR OF SAFETY CALCULATION	154
C.9.1 Internal Stability Calculation	154
C.9.2 Summary	161
C.10 CONCLUSIONS.....	161
APPENDIX D — NUMERICAL MODELING	163
D.1 PRELIMINARY WORK	163
D.1.1 Geogrid Pullout Simulation	163
D.1.2 Modeling Issues	165
D.2 ANALYSIS DETAILS	166
D.2.1 Soil	166
D.2.2 Structures	168
D.2.3 Model Configuration	169
D.2.4 Initial Stress State and Modeling Sequence	171
D.3 ANALYSIS RESULTS	172
D.3.1 Geogrid Strain Behavior	172
D.3.2 MSE/Shoring Interface Pressure Behavior	172
D.3.3 Failure Characteristics	178
D.4 CONCLUSIONS	178
APPENDIX E — RESULTS OF GEOGRID PULLOUT SIMULATION	183
E.1 MEDIUM MESH COARSENESS.....	183
E.2 VERY FINE MESH COARSENESS	190
GLOSSARY OF TERMS.....	197
ACKNOWLEDGEMENTS	205
REFERENCES.....	207

LIST OF FIGURES

Figure 1.	Diagram. Generic cross section of an SMSE wall system.....	6
Figure 2.	Flow chart. Design methodology for SMSE wall systems.....	8
Figure 3.	Photo. El Portal Road re-construction.....	11
Figure 4.	Photo. Compound wall construction at Zion National Park.....	12
Figure 5.	Flow chart. Flow chart for assistance in SMSE wall selection.....	13
Figure 6.	Diagram. Proposed geometry of MSE wall component of an SMSE wall system.....	22
Figure 7.	Diagram. Alternate proposed geometry for MSE wall component of an SMSE wall system.....	23
Figure 8.	Diagram. Frictional connection options for an SMSE wall system.....	25
Figure 9.	Diagram. Mechanical connection options for an SMSE wall system.....	26
Figure 10.	Diagram. Stepped shoring wall interface.....	27
Figure 11.	Diagram. Conceptual internal drainage for SMSE wall system.....	28
Figure 12.	Diagram. Ideal boring layout for SMSE wall system design.....	30
Figure 13.	Diagram. SMSE wall system failure modes.....	34
Figure 14.	Diagram. Location of potential failure surface for internal stability design of MSE wall component with extensible reinforcements.....	38
Figure 15.	Diagram. Location of potential failure surface for internal stability design of MSE wall component with inextensible reinforcements.....	38
Figure 16.	Chart. Variation in lateral stress ratio coefficients with depth in an MSE wall. ⁽¹⁾	40
Figure 17.	Diagram. Battered MSE wall facing.....	41
Figure 18.	Diagram. Distribution of stress from concentrated vertical load F_V for internal and external stability calculations.....	42
Figure 19.	Diagram. Free-body diagram for calculation of required tensile capacity in the resistant zone.....	44
Figure 20.	Diagram. Calculation of vertical stress at foundation level.....	49
Figure 21.	Chart. Modified bearing capacity factors for footing adjacent to sloping ground. ⁽¹⁾	50
Figure 22.	Diagram. Conceptual failure surface and design methodology assuming zero interface shear strength.....	55
Figure 23.	Diagram. Conceptual failure surface to evaluate stability along shoring/MSE interface.....	57
Figure 24.	Diagram. Conceptual global stability failure surface.....	58
Figure 25.	Illustration. Illustration of design example.....	67
Figure 26.	Calculation. Reinforcement rupture calculation for the design example.....	73
Figure 27.	Calculation. Required total tensile capacity of MSE reinforcements for design example.....	74
Figure 28.	Calculation. Pullout resistance calculation for design example.....	75
Figure 29.	Screenshot. Interface stability check for the design example.....	76
Figure 30.	Illustration. Staged construction procedures for the GRS-RW system. ⁽⁴³⁾	90
Figure 31.	Illustration. Profile of a multi-anchored wall (A) and plan view of the reinforcement (B). ⁽⁴⁵⁾	93

Figure 32.	Illustration. A multi-nailing shoring system combined with MSE construction. ⁽⁴⁶⁾	94
Figure 33.	Diagram. Dimensioning for MSE wall with variable reinforcement lengths. ⁽²⁾	96
Figure 34.	Graph. Particle size distribution for Monterey No. 30 sand used for Phase I centrifuge modeling. ⁽⁴⁹⁾	105
Figure 35.	Graph. Gradation of mortar sand used for Phase II centrifuge testing.	106
Figure 36.	Schematic. Schematic of centrifuge model test set-up. ⁽⁴⁹⁾	107
Figure 37.	Illustration. Phase II centrifuge model configuration.	111
Figure 38.	Photo. Centrifuge test series 2 at 37g acceleration.	113
Figure 39.	Photo. Centrifuge test series 2 at 38g acceleration.	113
Figure 40.	Photo. Centrifuge test series 2 at 41g acceleration.	114
Figure 41.	Schematic. Test wall plan view.	120
Figure 42.	Schematic. Typical field-scale test wall cross section with unconnected system.	121
Figure 43.	Schematic. Typical field-scale test wall cross section with connected system.	122
Figure 44.	Schematic. Connection detail for connected wall system.	123
Figure 45.	Photo. Reinforced fill compaction and retained fill placement.	123
Figure 46.	Photo. Nuclear density gage testing of reinforced fill zone.	124
Figure 47.	Schematic. Plan view of shoring beam connection to pit wall.	125
Figure 48.	Photo. Installation of shoring beam.	125
Figure 49.	Schematic. Tensar® welded wire facing unit.	126
Figure 50.	Photo. Geogrid installation.	126
Figure 51.	Schematic. Instrumented wall section.	128
Figure 52.	Photo. Strain gage installed on uniaxial geogrid.	129
Figure 53.	Photo. Earth pressure cells, Model 4800 (left) and Model 4810 (right).	129
Figure 54.	Photo. Inclinometers installed at the face of the MSE wall.	130
Figure 55.	Photo. Total station surveying of footing deflection.	130
Figure 56.	Photo. LVDT instrumentation installation.	131
Figure 57.	Photo. Potentiometer installation showing connection to vertical reference.	131
Figure 58.	Photo. Potentiometer wire connection to welded wire facing.	132
Figure 59.	Graph. Footing settlement measurements recorded during dead loading.	133
Figure 60.	Photo. Field-scale test wall load frame and jack set-up.	133
Figure 61.	Photo. Development of slack in geogrid reinforcement during wall loading.	134
Figure 62.	Graph. Strain measurements in geogrid, connected wall system.	135
Figure 63.	Graph. Strain measurements in geogrid, unconnected wall system.	136
Figure 64.	Graph. Average measured strain versus applied surcharge pressure.	137
Figure 65.	Graph. Measured lateral earth pressures for the connected and unconnected wall systems.	138
Figure 66.	Graph. Measured vertical pressures for the connected and unconnected wall systems.	140
Figure 67.	Graph. Measured versus applied vertical pressures excluding overburden.	141
Figure 68.	Graph. Calculated lateral earth pressure coefficient.	142

Figure 69.	Graph. Measured cumulative displacement of MSE wall face.....	143
Figure 70.	Graph. Measured cumulative displacement of shoring wall.....	144
Figure 71.	Graph. Measured settlement of load footings using total station.....	145
Figure 72.	Graph. Measured horizontal displacement of load footings using total station.....	146
Figure 73.	Graph. Comparison of settlement measurements obtained using total station and level.....	147
Figure 74.	Graph. Average vertical settlement of load footings measured using LVDT.....	148
Figure 75.	Graph. Potentiometer measurements for the connected and unconnected wall systems.....	149
Figure 76.	Graph. Comparison of centrifuge reinforcement tears to field-scale test wall strain gage locations.....	152
Figure 77.	Graph. Comparison of theoretical active failure wedge to actual failure geometry.....	153
Figure 78.	Calculation. Calculation of vertical stress due to footing load for test wall.....	156
Figure 79.	Calculation. Reinforcement rupture calculation for test wall.....	157
Figure 80.	Calculation. Calculation of required pullout capacity for test wall.....	159
Figure 81.	Calculation. Calculation of pullout resistance for test wall.....	160
Figure 82.	Diagram. Geogrid pullout simulation model set-up.....	164
Figure 83.	Graph. Stress-strain comparison over small strain range.....	167
Figure 84.	Graph. Stress-strain comparison over large strain range.....	167
Figure 85.	Diagram. PLAXIS field-scale test wall model configuration.....	170
Figure 86.	Screenshot. PLAXIS model mesh discretization.....	171
Figure 87.	Graph. Calculated strains in geogrid layers over field-scale test load range.....	173
Figure 88.	Graph. Calculated strains in geogrid layers over model load range.....	174
Figure 89.	Graph. Lateral pressures recorded at tracking points for footing pressures up to 350 kPa.....	175
Figure 90.	Graph. Vertical pressures recorded at tracking points for footing pressures up to 350 kPa.....	176
Figure 91.	Graph. Lateral pressures recorded at pressure tracking points.....	177
Figure 92.	Graph. Vertical pressures recorded at pressure tracking points.....	177
Figure 93.	Screenshot. Principal stress directions at footing loading of 50 kPa.....	179
Figure 94.	Screenshot. Principal stress directions prior to failure (footing loading = 1,050 kPa).....	180
Figure 95.	Screenshot. Relative shear contours at footing loading of 50 kPa.....	181
Figure 96.	Screenshot. Relative shear contours prior to failure (footing loading = 1,050 kPa).....	182
Figure 97.	Screenshot. Plastic point development at displacement of 0.005 m, medium mesh.....	183
Figure 98.	Screenshot. Geogrid development length at displacement of 0.005 m, medium mesh.....	183
Figure 99.	Screenshot. Plastic point development at displacement of 0.010 m, medium mesh.....	184

Figure 100.	Screenshot. Geogrid development length at displacement of 0.010 m, medium mesh.....	184
Figure 101.	Screenshot. Plastic point development at displacement of 0.015 m, medium mesh.....	185
Figure 102.	Screenshot. Geogrid development length at displacement of 0.015 m, medium mesh.....	185
Figure 103.	Screenshot. Plastic point development at displacement of 0.02 m, medium mesh.....	186
Figure 104.	Screenshot. Geogrid development length at displacement of 0.02 m, medium mesh.....	186
Figure 105.	Screenshot. Plastic point development at displacement of 0.05 m, medium mesh.....	187
Figure 106.	Screenshot. Geogrid development length at displacement of 0.05 m, medium mesh.....	187
Figure 107.	Screenshot. Plastic point development at displacement of 0.10 m, medium mesh.....	188
Figure 108.	Screenshot. Geogrid development length at displacement of 0.10 m, medium mesh.....	188
Figure 109.	Screenshot. Plastic point development at displacement of 0.20 m, medium mesh.....	189
Figure 110.	Screenshot. Geogrid development length at displacement of 0.20 m, medium mesh.....	189
Figure 111.	Screenshot. Plastic point development at displacement of 0.005 m, very fine mesh.....	190
Figure 112.	Screenshot. Geogrid development length at displacement of 0.005 m, very fine mesh.....	190
Figure 113.	Screenshot. Plastic point development at displacement of 0.010 m, very fine mesh.....	191
Figure 114.	Screenshot. Geogrid development length at displacement of 0.010 m, very fine mesh.....	191
Figure 115.	Screenshot. Plastic point development at displacement of 0.015 m, very fine mesh.....	192
Figure 116.	Screenshot. Geogrid development length at displacement of 0.015 m, very fine mesh.....	192
Figure 117.	Screenshot. Plastic point development at displacement of 0.02 m, very fine mesh.....	193
Figure 118.	Screenshot. Geogrid development length at displacement of 0.02 m, very fine mesh.....	193
Figure 119.	Screenshot. Plastic point development at displacement of 0.05 m, very fine mesh.....	194
Figure 120.	Screenshot. Geogrid development length at displacement of 0.05 m, very fine mesh.....	194
Figure 121.	Screenshot. Plastic point development at displacement of 0.1 m, very fine mesh.....	195
Figure 122.	Screenshot. Geogrid development length at displacement of 0.1 m, very fine mesh.....	195

TABLE OF CONTENTS

Figure 123. Screenshot. Plastic point development at displacement of 0.2 m, very fine mesh.....	196
Figure 124. Screenshot. Geogrid development length at displacement of 0.2 m, very fine mesh.....	196

LIST OF TABLES

Table 1.	Select granular fill gradation example specification.....	20
Table 2.	Embedment depths (d) for MSE walls. ⁽²⁾	26
Table 3.	Interface friction angles. ⁽²⁷⁾	56
Table 4.	Recommended SMSE wall construction tolerances.....	80
Table 5.	Summary of SMSE wall system design recommendations	84
Table 6.	Centrifuge scaling relations. ^(57,58)	104
Table 7.	Unconfined tensile strengths of the reinforcement.....	104
Table 8.	Summary of Phase I centrifuge test models.....	109
Table 9.	Centrifuge model parameters compared to prototype parameters.....	110
Table 10.	Comparison of centrifuge model and prototype footing pressures.....	110
Table 11.	Summary of Phase I centrifuge test results.....	112
Table 12.	Specification summary for test wall instrumentation.....	127
Table 13.	Results of geogrid pullout simulation.....	164
Table 14.	Soil model parameters.....	168
Table 15.	Modeling parameters for geogrid.....	168
Table 16.	Modeling parameters for MSE facing units.....	168
Table 17.	Modeling parameters for loading footing.....	169

LIST OF ABBREVIATIONS AND SYMBOLS

AASHTO	-	American Association of State Highway and Transportation Officials
A_f	-	area of load footing
A_M	-	maximum horizontal acceleration
ASTM	-	American Society for Testing and Materials
b	-	gross width of the strip, sheet or grid; or bench width
b_f	-	length of load footing measured perpendicular to wall face
B	-	width of MSE wall measured from wall face
c_f	-	cohesion of foundation soil
C	-	reinforcement effective unit perimeter
C_c	-	coefficient of consolidation
C_u	-	uniformity coefficient (D_{60}/D_{10})
C_v	-	compression index
d	-	foundation or toe embedment depth of MSE wall
D_f	-	footing embedment depth
D_r	-	relative density
D_I	-	diameter of influence from footing load
D_{10}	-	particle size which 10 percent of material passes
D_{30}	-	particle size which 30 percent of material passes
D_{60}	-	particle size which 60 percent of material passes
DOT	-	Department of Transportation
e	-	eccentricity
EA	-	axial stiffness
EI	-	bending stiffness
E_{50}^{ref}	-	reference secant modulus for deviatoric loading
E_{oed}^{ref}	-	reference secant modulus for primary compression
E_{ur}^{ref}	-	reference secant modulus for unloading/reloading
F	-	maximum tensile force
F^*	-	pullout resistance factor
F_H	-	concentrated horizontal load
F_V	-	concentrated vertical load
F_q	-	embedment bearing capacity factor
F_{PO}	-	pullout resistance
FHWA	-	Federal Highway Administration
FLH	-	Federal Lands Highway
FS	-	factor of safety to account for uncertainties
FS_{bc}	-	factor of safety against bearing capacity failure
FS_c	-	factor of safety against compound failure
FS_{cs}	-	factor of safety with regard to connection strength

FS_{ex}	–	factor of safety against external instability
FS_g	–	factor of safety against global failure
FS_{is}	–	factor of safety against interface shear instability
FS_{ot}	–	factor of safety against overturning failure
FS_p	–	factor of safety against MSE reinforcement pullout failure
FS_{PO}	–	factor of safety against soil nail pullout
FS_r	–	factor of safety against reinforcement rupture
FS_{sc}	–	factor of safety against internal shear failure
FS_{sl}	–	factor of safety against base sliding
FS_t	–	nail tensile capacity factor of safety
g	–	gravitational acceleration
H	–	horizontal distance
H	–	vertical wall height
H_s	–	slope height for bearing calculation
HDPE	–	high density polyethylene
i	–	slope inclination angle
kN	–	kiloNewton
K	–	the horizontal force coefficient acting on the back of the wall face
K_a	–	active lateral earth pressure coefficient
K_r	–	lateral earth pressure coefficient
K_r/K_a	–	lateral stress ratio
kPa	–	kiloPascal
L	–	length of reinforcement
L_B	–	reinforcement length at base of MSE wall
L_{ei}	–	length of embedment in the resisting zone at the i^{th} reinforcement level
L_f	–	length of load footing
L_T	–	reinforcement length at top of MSE wall
L_w	–	length of truncated failure wedge; wall length
L_z	–	nail length at depth, z
LRFD	–	load and resistance factor design
LVDT	–	linear variable displacement transducer
m	–	meter(s)
mm	–	millimeter(s)
m	–	power for stress-level dependency of stiffness
M	–	mass of active soil
MSE	–	mechanically stabilized earth
N	–	coefficient of gravitational acceleration
N_1	–	reaction force normal to failure surface
N_2	–	reaction force normal to shoring wall

N_{cq}	–	dimensionless bearing capacity factor
$N_{\gamma q}$	–	dimensionless bearing capacity factor
N_s	–	slope stability factor
NCMA	–	National Concrete Masonry Association
OSHA	–	Occupational Safety and Health Association
P_{AE}	–	dynamic horizontal thrust
P_D	–	driving force
P_{IR}	–	horizontal inertia force
P_o	–	lateral reactionary force
P_R	–	resisting force
p^{ref}	–	reference pressure
PI	–	plasticity index
PVC	–	polyvinyl chloride
q	–	uniform surcharge load
Q	–	ultimate nail pullout resistance
q_a	–	allowable bearing capacity
q_{ult}	–	ultimate bearing capacity
R_c	–	reinforcement coverage ratio (b/s_h)
R_f	–	failure ratio
S_1	–	shear resistance along the failure surface
S_2	–	shear resistance along the shoring wall
s_h	–	center-to-center horizontal spacing between strips, sheets or grids for MSE wall
S_H	–	center-to-center horizontal spacing between nails for soil nail wall
SP	–	poorly-graded sand
s_v	–	vertical spacing between MSE reinforcements
S_V	–	center-to-center vertical spacing between nails for soil nail wall
S_t	–	spacing of transverse bar of grid reinforcements
SCR	–	Supplemental Contract Requirement
SMSE	–	shored mechanically stabilized earth
t	–	thickness of the transverse bar of grid reinforcement
T	–	reinforcement tensile strength
$T_{allowable}$	–	allowable strength (force per unit width) of reinforcement
T_i	–	maximum tension per unit width at i^{th} reinforcement level
T_n	–	nominal or ultimate nail tendon tensile strength
T_{max}	–	required pullout resistance
TFHRC	–	Turner Fairbanks Highway Research Center
USCS	–	Unified Soil Classification System

V	—	vertical distance
v	—	vertical component of shoring wall batter
w	—	width of load footing measured parallel to wall face
W	—	weight of the active wedge or reinforced block
W_f	—	width of load footing
x	—	distance to center of footing measured from face of MSE wall
z	—	depth below top of wall
γ	—	unit weight
γ_f	—	unit weight of foundation soil
ϕ	—	friction angle
ϕ'	—	effective friction angle
ϕ_f	—	friction angle of foundation soil
ϕ_{PS}	—	plane strain friction angle
ϕ_{TX}	—	triaxial shear friction angle
α	—	scale effect correction factor; aspect ratio
α_β	—	bearing factor for passive resistance
β	—	internal angle of truncated failure wedge
β_s	—	slope angle measured from horizontal
δ	—	inclination of MSE wall facing measured from horizontal starting in front of the wall
δ_i	—	interface friction angle
ψ	—	angle of the failure surface measured from horizontal
ψ_d	—	dilatancy angle
ν_{ur}	—	Poisson's ratio for unloading/reloading
ρ	—	soil-reinforcement interaction friction angle
$\Delta\sigma_h$	—	concentrated horizontal surcharge load
$\Delta\sigma_v$	—	concentrated vertical surcharge load
σ_h	—	horizontal stress
σ_v	—	vertical stress
σ_{vi}	—	overburden pressure at the i^{th} reinforcement level
σ_z	—	horizontal pressure at depth, z
$\sigma_{tension}$	—	tensile strength
σ_3	—	confining stress